

2558A

AC Voltage Current Standard

SIMPLE STANDALONE SOLUTION
FOR CALIBRATING METERS, CLAMPS AND CTs



Easy Operation

A dial
for each function

High Accuracy

0.04% AC Voltage
0.05% AC Current

Wide Output Range

1.00 mV
to **1200.0 V**
1.00 mA
to **60.00 A**

For more information, go to
tmi.yokogawa.com
Test & Measurement Instruments




1-Year Warranty 

Reliable and Simple Operation

New AC Voltage Current Standard from "YOKOGAWA"

The wide output ranges of 1.00 mV to 1200.0 V* AC and 1.00 mA to 60.00 A* AC mean that the 2558A is the instrument of choice for the cost effective calibration of AC analog meters. Rotary controls and a range of computer interfaces enable the 2558A to be intuitively operated through the front panel or controlled by an ATE system.

*With the deviation function, the maximum output is 1440 V and 72 A.

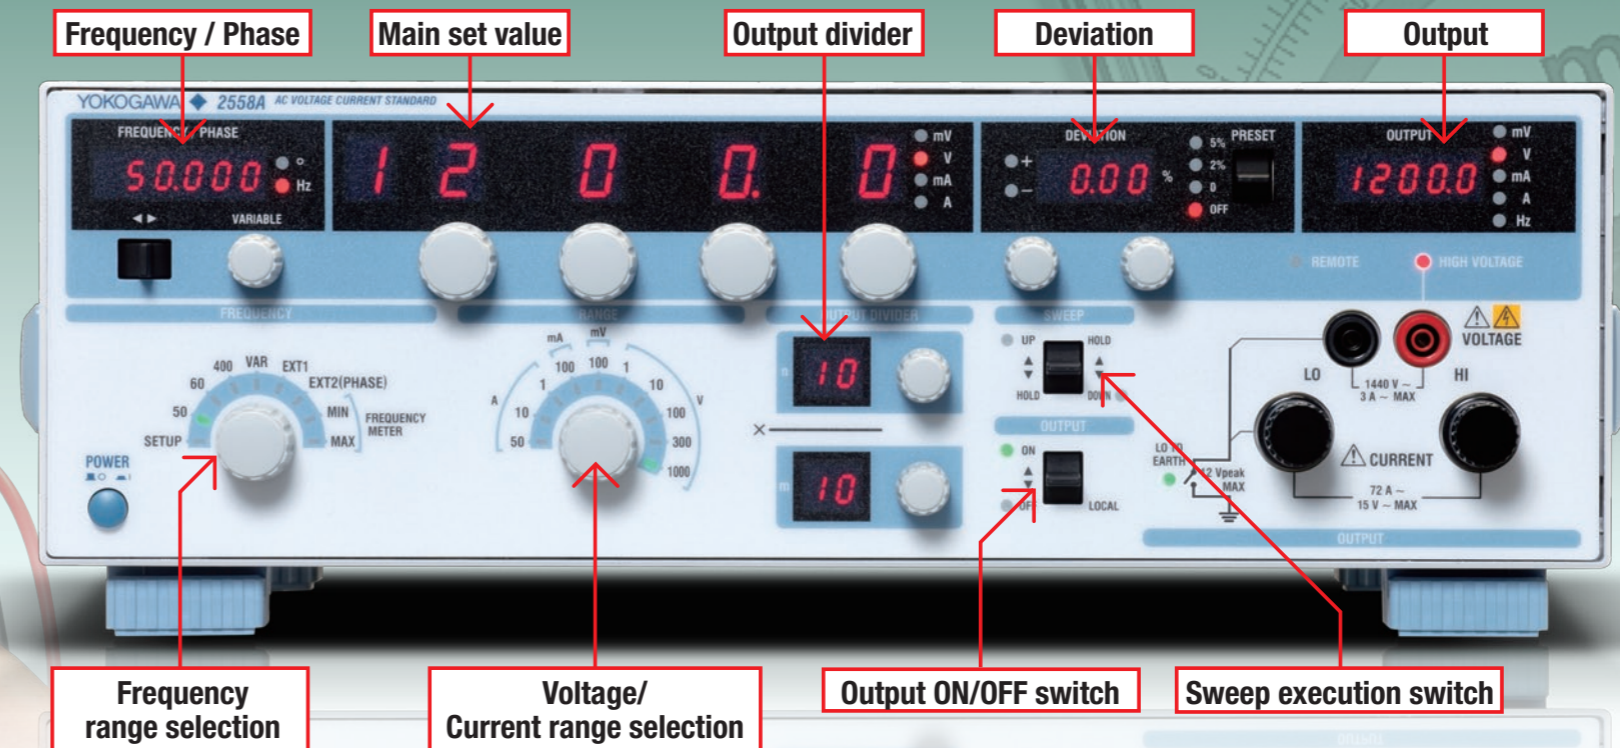

Intuitive operation

Dials and switches are provided for each digit and function, and traditional 7-segment LEDs provide clear visibility.

Sweep (Voltage/Current/Frequency*1)

With a flick of a switch, the output can be swept from 0% to 120% of the main set value with sweep times of 8*2, 16, 32 or 64 seconds.

*1 The range of frequency sweep can be set.

*2 Firmware version 1.04 or later.

Output Divider

Linearity tests can be simply performed by dividing the output into steps. For example, a setting of 4 will generate steps of 25, 50, 75 and 100% of the set output value.

Direct readout of the deviation

When the deviation dials are adjusted to check the full scale value on the meter, the deviation from the main output setting is displayed as a % of full scale.

Digital display of output

The actual output value is displayed. It is therefore unnecessary to calculate the output value from the main, divider and deviation settings.

You can confirm that the output is stable and how it corresponds to the target meter's reading.

Common current output terminals

The same output terminals are used for all current ranges. Test times are therefore reduced by avoiding the need to change the wiring for meters which have different ranges.

High accuracy

AC voltage : ±0.04 %
AC current : ±0.05 %

More than sufficient to calibrate meters with class 0.1% accuracy.

	10 to 120 % of range		
	± (% of setting + % of range)		
	50/60 Hz	40 ≤ f ≤ 400 Hz	400 < f ≤ 1 kHz
AC voltage	0.03 + 0.01*	0.05 + 0.01	0.10 + 0.02
AC current	0.04 + 0.01*	0.06 + 0.01	0.12 + 0.02

* Add 0.1% of range when output is 120% to 144% of range

	1 to 10 % of range		
	± (% of range)		
	50/60 Hz	40 ≤ f ≤ 400 Hz	400 < f ≤ 1 kHz
AC voltage	0.013	0.015	0.03
AC current	0.014	0.016	0.032

High stability

AC voltage/current : ±50 ppm/h

± (20 ppm of range + 30 ppm of range)/h
Perform measurements with high repeatability over time

Wide output range

AC voltage : 1.00 mV to 1200.0 V
AC current : 1.00 mA to 60.00 A

6 voltage ranges (100 m/1/10/100/300/1000 [V])
4 current ranges (100 m/1/10/50 [A])

The generation range is 0 to 144 % of range

Ex. Set for the output

1. Select the range
2. Main setting : Available for 0 to 120 % of the range
3. Output divider : n & m (n/m of main set value)
m = The number of required calibration points
if the main set value = 100V, m = 5 and n = 1, the output will be 20 V
4. Deviation : Available for ± 20 % of the main setting

Max. output current is "72A" at the 50 A range

Main setting : 60 A
Output divider : n = m
Deviation : - 20%

Wide frequency range

40 to 1000 Hz
(Frequency accuracy : ±50 ppm)

The 2558A provides fixed frequencies of 50/60 Hz (commercial) and 400 Hz (marine and aviation), as well as variable frequencies from 40 to 1000 Hz.

The high frequency accuracy of the 2558A (50 ppm) also enables it to be used to calibrate frequency meters.

Multiple 2558As can be synchronized using the internal phase shifter. This means that two 2558As can be used as accurate sources of voltage and current for calibrating power meters.

2558A


AC Voltage Current Standard



Power calibration

A power calibration system can be created by using two 2558As (one each for AC voltage and AC current) together with a Yokogawa WT3000E power analyzer as the reference. One of the 2558As acts as the master unit and provides the synchronizing oscillator signal. The required power factor is set by adjusting the phase shifter on the slave unit and monitoring the result on the WT3000.


A 3 phase power calibrator system can be simply built by adding further 2558As.

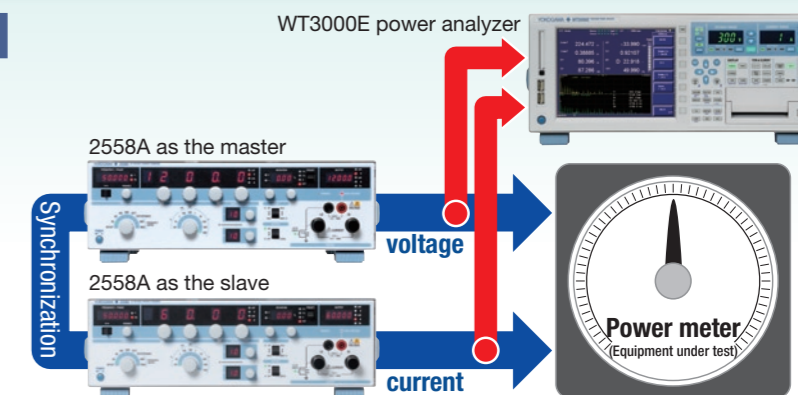

Higher current output

To generate higher current than 72 A, two 2558As can be connected to double the output to 144 A.

- Condition :
- Accuracy, stability, temperature coefficient is the sum of the individual units.
 - 50/60 Hz only.

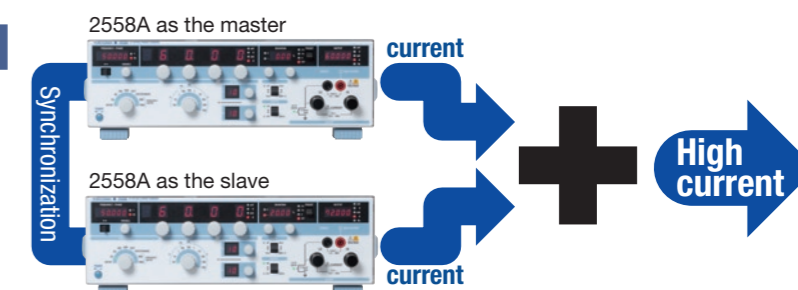


Calibration and test for meters

The 2558A provides specific functions to enable meters to be calibrated accurately and efficiently.

Using the output divider and deviation


Calibrating two or more points is quick and simple. It is only necessary to preselect the number of required calibration points with the lower divider control and then use the upper control to step the output to the next calibration point. The deviation settings will then enable the output value and error of each calibration point to be displayed directly.

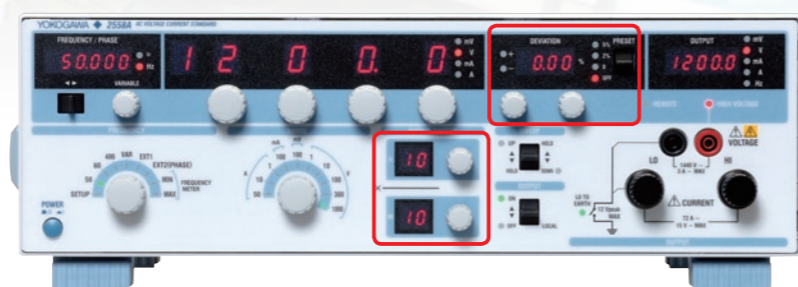

Using the output divider and deviation preset

The deviation preset control can be used to move the output value in small increments (2 or 5% of the step between calibration points).

This means that it is possible to finely approach the target calibration point, either from a lower value or a higher one, without exceeding it. This is particularly useful when the friction (hysteresis) of the moving part needs to be taken into consideration. In this case the point is calibrated twice, once from a lower value and once more from a higher value and the final calibration result is the average of the two.

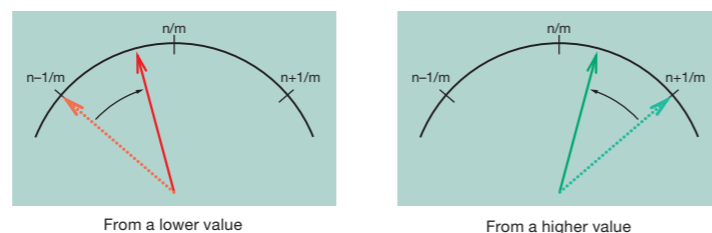


Using sweep

Needle sticking tests can be performed with high repeatability. It is possible to stop at any point and sweep around it in fine detail.

Use existing 2558 programs

The 2558A is backwardly compatible with the previous 2558 model. The new 2558A supports a 2558 command mode, which means that you can switch from the 2558 to the 2558A without modifying your program. It is also possible to mix 2558s and new 2558As in the same system.*


* Programs may need to be modified due to the improvement in the response time etc.

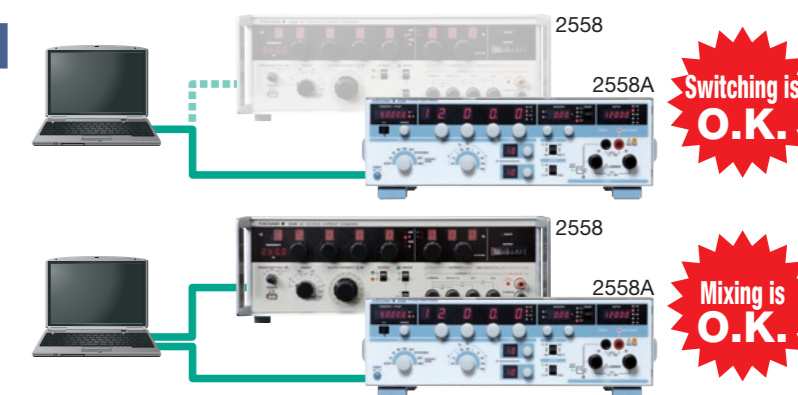

Comparison with the 2558

		2558A	2558
AC Voltage	Output range of the specified accuracy	1.00 mV to 1200.0 V	1.00 mV to 1200.0 V
	Accuracy (50/60 Hz)	± 400 ppm	± 950 ppm
	Frequency of the specified accuracy	40 to 1000 Hz	50 / 60 / 400 Hz
AC Current	Output range of the specified accuracy	1.00 mA to 60.00 A	1.00 mA to 60.00 A
	Accuracy (50/60 Hz)	± 500 ppm	± 950 ppm
	Frequency of the specified accuracy	40 to 1000 Hz	50 / 60 / 400 Hz
Frequency	Output range	40 to 1000 Hz	40 to 500 Hz
	Accuracy	± 50 ppm	± 1%
Max. output		Approx. 36 VA (60 A/0.6 V)	Approx. 36 VA (60 A/0.6 V)
Stability		± (20 ppm of setting + 30 ppm of range)/h	± (0.03% of range)/h
Dimension (mm)		426 (W) × 132 (H) × 400 (D)	439 (W) × 149 (H) × 415 (D)

Rear Panel

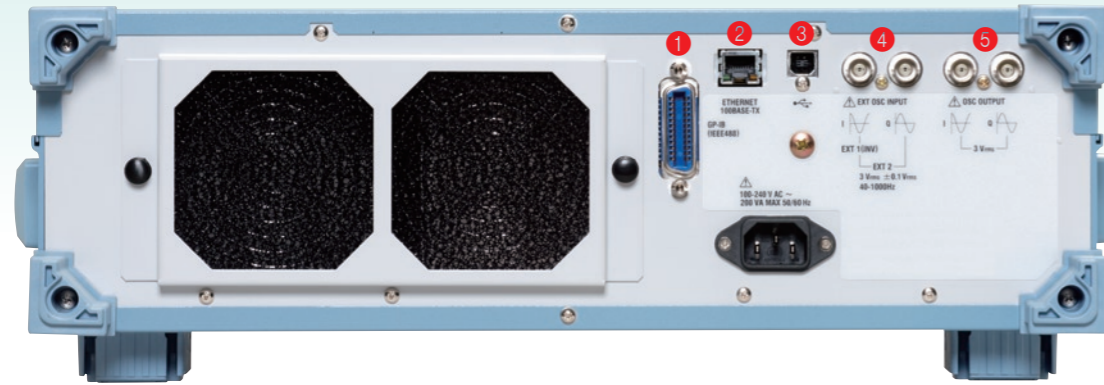

- 1 GP-IB interface (optional, /C1)
- 2 Ethernet
- 3 USB interface (for PC connection)
- 4 Input terminals for synchronized operation
- 5 Output terminals for synchronized operation

Specification

Output

Range	Output range	Specified output range*	Resolution	Maximum output
100 mV	0 to 144.00 mV	1 to 120.00 mV	10 μV	—
1 V	0 to 1.4400 V	0.01 to 1.2000 V	100 μV	0.5 A or more
10 V	0 to 14.400 V	0.1 to 12.000 V	1 mV	Approx. 3 A
100 V	0 to 144.00 V	1 to 120.00 V	10 mV	Approx. 0.3 A
300 V	0 to 432.0 V	3 to 360.0 V	100 mV	Approx. 0.1 A
1000 V	0 to 1440.0 V	10 to 1200.0 V	100 mV	Approx. 6 mA
100 mA	0 to 144.00 mA	1 to 120.00 mA	10 μA	Approx. 15 V
1 A	0 to 1.4400 A	0.01 to 1.2000 A	100 μA	Approx. 15 V
10 A	0 to 14.400 A	0.1 to 12.000 A	1 mA	Approx. 3 V
50 A	0 to 72.00 A	0.5 to 60.00 A	10 mA	Approx. 0.6 V

Condition Frequency : Internal oscillator
 Temperature/Humidity : 23 ± 3 °C/20 to 80 %RH
 Add the temp. coefficient at 5 to 20°C, 26 to 40°C

Accuracy

Range	Upper : 180 days Lower : 1 year			1% to 10% of range		
	± (% of setting + % of range)			± (% of range)		
	50/60 Hz	40 Hz ≤ f ≤ 400 Hz	400 Hz < f ≤ 1 kHz	50/60 Hz	40 Hz ≤ f ≤ 400 Hz	400 Hz < f ≤ 1 kHz
100 mV						
1 V						
10 V	0.03 + 0.01*	0.05 + 0.01	0.10 + 0.02	0.013	0.015	0.030
100 V	0.04 + 0.01*	0.06 + 0.01	0.11 + 0.02	0.014	0.016	0.031
300 V						
1000 V						
100 mA						
1 A	0.04 + 0.01*	0.06 + 0.01	0.12 + 0.02	0.014	0.016	0.032
10 A	0.055 + 0.01*	0.075 + 0.01	0.135 + 0.02	0.0155	0.0175	0.0335
50 A						

* Add 0.1% of range when output is 120% to 144% of range

Stability

± (20 ppm of setting + 30 ppm of range)
 Condition Output : 1 to 120% of range
 Frequency : Internal oscillator
 Temperature/Humidity : 23±3°C / 20 to 80%RH
 Time : 1 min. to 1 hour after output ON

Temperature Coefficient (5 to 20°C, 26 to 40°C)

50/60 Hz : ±(30 ppm of setting/°C)
 Other : ±(50 ppm of setting/°C)

Distortion Factor

Voltage output : 0.07% or less
 Current output : 0.18% or less
 Condition Output : 40 to 120% of range*
 Load : Resistance only
 20% of the max. output or less
 (Current at the voltage output,
 or voltage at the current output)

Frequency : 40 to 1000 Hz
 * 40 to 144% of range when frequency is 50 or 60 Hz

Specification

AC Voltage Current Standard 2558A

Frequency range

Accuracy (internal) : ± 50 ppm (180 days)
 ± 100 ppm (1 year)
 Mode : Internal / External / FREQUENCY METER
 Internal : 50 / 60 / 400 Hz
 VAR (40 to 1000 Hz, 0.001 Hz resolution)
 External : EXT1 / EXT2
 (Use the terminals for the synchronized operation)
 FREQUENCY METER : MIN/MAX
 Range : 20 to 1000 Hz
 Resolution : 0.001 Hz
 Sweep, output divider and deviation functions are used for the frequency.

Sweep

Target : Voltage / Current / Frequency
 Speed : Approx. 8*/16/32/64 sec. selectable
 During 0 to 100%, 100 to 0% of setting
 * Firmware version 1.04 or later.

Output divider

Target : Voltage / Current / Frequency
 Denominator : m 4 to 15
 Numerator : n 0 to 15 (n ≤ m)

Deviation

Target : Voltage / Current / Frequency
 Variable range : ±20.00%
 Operation : Two dials
 Resolution of the first dial : 0.2% of the main setting
 Resolution of the second dial : 0.01% of the main setting
 Deviation preset : OFF / 0 / 2% / 5%

Output terminal

Type Voltage : Plug-in terminal (safety terminal)
 Current : Large binding post
 Selectable LO terminal to earth or floating.
 Max. floating voltage to earth : 12 Vpk

Display

Main setting : 5 digits LED
 Output Divider : 2 digits LED (m and n)
 Deviation : 4 digits LED
 Output : 5 digits LED
 Frequency/Phase : 6 digits LED

SETUP

Setting : Communication, Beep sound, Sweep speed, Earth/Floating
 Status : Self test, Error log, Product Information

External I/O

Sync. Terminals (two input terminals and two output terminals)
 I/O voltage : 3±0.1 Vrms, 2 phase sine wave
 Frequency : 40 to 1000 Hz
 Input resistance : Approx. 1 MΩ
 Output resistance : Approx. 50 Ω

USB PC interface (for PC connection)

Connector : Type B connector (receptacle)
 Electrical and mechanical specifications : Complies with USB Rev. 2.0
 Supported transfer modes : High Speed, Full Speed

Ethernet interface

Connector : RJ-45 connector
 Electrical and mechanical specifications : Confirms to the IEEE 802.3
 Transmission methods : 100 BASE-TX / 10 BASE-T

GP-IB interface (/C1 optional)

Electrical and mechanical specifications : Complies with IEEE St'd 488-1978
 Functional specifications : SH1, AH1, T6, L4, SR1, RL1, PP0, DC1, DT1, C0
 Address : 0 to 30

General specifications

Warm-up time : Approx. 30 minutes
 Operating environment : Temperature : 5 to 40°C
 Humidity : 20 to 80%RH (no condensation)
 Attitude 2000 m or less
 Installation locations : Indoors
 Storage environment : Temperature -15 to 60°C
 Humidity 20 to 80%RH (no condensation)
 Rated power supply voltage : 100 to 120 VAC / 200 to 240 VAC
 Allowable power supply voltage fluctuation range : 90 to 132 VAC / 180 to 264VAC
 Rated power supply frequency : 50/60 Hz
 Allowable power supply frequency fluctuation range : 48 to 63 Hz
 Max. power consumption : 200 VA
 Weight : Approx. 20 kg
 Dimensions : 426(W) x 132(H) x 400(D) mm

Accessories



B8506ZK
Measurement lead set
 2 pieces (red and black) in 1 set,
 length: 1.00 m Used in combination with the
 B8506ZL, 701902, 758921, 758922, or 758929.
 Rating: 1500 V CAT I/19 A



B8506WA
Measurement lead set
 2 pieces (red and black) in 1 set,
 length : 1.5 m, Rating : 80 A



758917
Measurement lead set
 2 pieces (red and black) in 1 set,
 length: 0.75 m Used in combination with the
 B8506ZL, 701902, 758921, 758922, or 758929.
 Rating: 1000 V CAT II/32 A



758922
Small Alligator clip adapter set
 Safety terminal (banana female)-to-alligator
 clip adapter 2 pieces (red and black) in
 1 set Rating: 300 V CAT II Connected to the
 B8506ZK, 758933, 758917, or 701901.



B8506ZL
Large Alligator clip adapter set
 Safety terminal (banana female)-to-alligator
 clip adapter 2 pieces (red and black) in
 1 set Rating: 1500 V CAT I Connected to the
 B8506ZK, 758933, 758917, or 701901.



758921
Fork terminal adapter set
 Two adapters (red and black) to a set. Used
 when attaching banana plug to binding post.



701902 / 701903
Safety BNC-BNC cable
 701902: Length 1 m, 1000 V CAT II
 701903: Length 2 m, 1000 V CAT II



758923
Safety terminal adapter set
 Spring-hold type (banana male) 2 pieces in
 1 set. Easy attachment/detachment of the
 cable.



758931
Safety terminal adapter set
 Screw-fastened type (banana male)
 2 pieces in 1 set. Comes with a B9317WD
 1.5 mm hexagonal wrench for fixing the
 cable in place.

* Wire diameter of cables that can connect to the adapter
 758923 Core wire diameter: 2.5 mm or less,
 insulation diameter: 5.0 mm or less
 758931 Core wire diameter: 1.8 mm or less,
 insulation diameter: 3.9 mm or less

Due to the nature of the product, it is possible for the user to come in contact with metal parts and receive electric shock. Exercise caution when using the product.

AC Voltage Current Standard 2558A

Model and Suffix Codes

Model	Suffix code	Description
2558A		AC Voltage Current Standard
Power cord	-D	UL/CSA standard, PSE
	-F	VDE standard
	-R	AS standard
	-Q	BS standard
	-H	GB standard
	-N	NBR standard
Option	/C1	GP-IB interface

Standard Accessories

Part name	Quantity
Power cord	1
Measurement lead set (B8506ZK)	1 set (red and black)
Measurement lead set (B8506WA)	1 set (red and black)
Large alligator clip adapter set (B8506ZL)	1 set (red and black)
Rubber leg cap	1 set (2)
User's manual	1 set

Rack Mount Kits

Model	Suffix code	Description
751535-E3	Rack mount kit	For EIA
751535-J3	Rack mount kit	For JIS

Optional Accessories

Model	Part name	Description
758933	Measurement lead set	Rating 1000 V, 1 m, 2 leads in a set
B8506ZK	Measurement lead set	Rating 1500 V, 1 m, 2 leads in a set
B8506WA	Measurement lead set	Rating 80 A, 1.5 m, 2 leads in a set
758917	Measurement lead set	Rating 1000 V, 75 cm, 2 leads in a set
758922	Alligator clip adapter set	Rating 300 V, 2 adapters in a set
758929	Alligator clip adapter set	Rating 1000 V, 2 adapters in a set
B8506ZL	Alligator clip adapter set	Rating 1500 V, 2 adapters in a set
758921	Fork terminal adapter set	Banana-fork adapter, 2 adapters in a set
701902	Safety BNC-BNC cable	1.0 m
701903	Safety BNC-BNC cable	2.0 m
758923	Safety terminal adapter set	Spring-hold type, 2 adapters in a set
758931	Safety terminal adapter set	Screw-fastened type, 2 adapters in a set

⚠ Due to the nature of this product, it is possible to touch its metal parts. Therefore, there is a risk of electric shock, so the product must be used with caution.
Actual allowable voltage is the lower of the voltages specified for the main unit and accessory.

This is a Class A instrument based on Emission standards EN61326-1 and EN55011, and is designed for an industrial environment. Operation of this equipment in a residential area may cause radio interference, in which case users will be responsible for any interference which they cause.


Yokogawa's Approach to Preserving the Global Environment

- Yokogawa's electrical products are developed and produced in facilities that have received ISO14001 approval.
- In order to protect the global environment, Yokogawa's electrical products are designed in accordance with Yokogawa's Environmentally Friendly Product Design Guidelines and Product Design Assessment Criteria.

NOTICE

- Before operating the product, read the user's manual thoroughly for proper and safe operation.

External dimensions

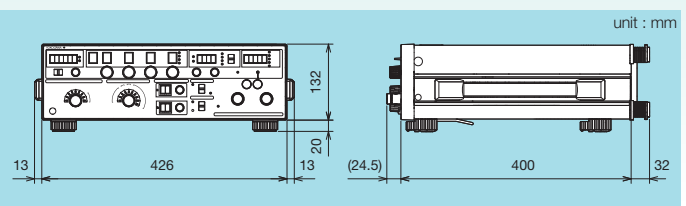

Related Product

2553A

Small and light Precision DC Calibrator

Accuracy Voltage: $\pm 0.0075\%$
Current: $\pm 0.0120\%$

Stability ± 15 ppm/h

Noise $2 \mu\text{Vrms}$

Resolution 5.5 digits, ± 120000 count display

Range Voltage: ± 32 V, Current: ± 120 mA
Thermocouple, RTD



2560A

High output Precision DC Calibrator

Accuracy Voltage: $\pm 0.0050\%$, Current: $\pm 0.0070\%$

Stability Voltage: ± 10 ppm/h, Current: ± 20 ppm/h

Resolution 5.5 digits, ± 120000 count display
6.5 digits, ± 1200000 count display
(in high resolution mode)

Range Voltage: ± 1224 V
Current: -12.24 A to $+36.72$ A
Thermocouple, RTD



YOKOGAWA

YMI-KS-MI-SE01

YOKOGAWA METERS & INSTRUMENTS CORPORATION

Global Sales Dept. /Phone: +81-422-52-6237 Facsimile: +81-422-52-6462
E-mail: tm@cs.jp.yokogawa.com

Subject to Change without notice.
Copyright © 2013, Yokogawa Meters & Instruments Corporation
[Ed: 04/b]
Printed in Japan, 602(KP)

YOKOGAWA CORPORATION OF AMERICA
YOKOGAWA EUROPE B.V.
YOKOGAWA SHANGHAI TRADING CO., LTD.
YOKOGAWA ELECTRIC KOREA CO., LTD.
YOKOGAWA ENGINEERING ASIA PTE. LTD.
YOKOGAWA INDIA LTD.
YOKOGAWA ELECTRIC CIS LTD.
YOKOGAWA AMERICA DO SUL LTDA.
YOKOGAWA AUSTRALIA PTY. LTD.
YOKOGAWA MIDDLE EAST & AFRICA B.S.C(oc)

Phone: +1-770-253-7000
Phone: +31-88-4641000
Phone: +86-21-6239-6363
Phone: +82-2-2628-3810
Phone: +65-6241-9933
Phone: +91-80-4158-6000
Phone: +7-495-737-7868
Phone: +55-11-5681-2400
Phone: +61-2-8870-1100
Phone: +973-17-358100

Facsimile: +1-770-254-0928
Facsimile: +31-88-4641111
Facsimile: +86-21-6880-4987
Facsimile: +82-2-2628-3899
Facsimile: +65-6241-2606
Facsimile: +91-80-2852-8656
Facsimile: +7-495-737-7869
Facsimile: +55-11-5681-4434
Facsimile: +61-2-8870-1111
Facsimile: +973-17-336100

<http://tmi.yokogawa.com/>